Accessory Book

Go To Table Of Contents

Sterilizer Accessory Parts Manual

FOR USE BY MIDMARK TRAINED TECHNICIANS ONLY

SF-1831

Part No. 004-0391-00 Rev. A (6/02)

Go To Table Of Contents

TABLE OF CONTENTS

Model	Description	Page
9A11500*	M9/M11 Sterilizer Printer	9A115
9A21500*	M11 Cassette Rack Assembly	9A215
9A22400*	M9 Deep Tray Assembly	9A224
9A22500*	M11 Deep Tray Assembly	9A225
9A22600*	M9/M11Pouch Rack	9A226
9A25800*	M4.9 Pouch Rack	9A258
9A25900*	M4.9 Sterilizer Printer	9A259
9A26000*	External Condensing Tank	9A260
9A30600*	M11 Large Cassette Tray	9A306
9A30700*	M4.9/M9/M11 Tray / Cass. Tool	9A307
COMMENTS		7-1
FAX ORDERING FORM		7-2

(†) = No Exploded Views Available.

© Midmark Corporation 2002 SF-1831 Rev3/03

Printed in U.S.A.

Return To Table Of Contents

© Midmark Corporation 1998 SF-1571 Rev. 2/02

Printed in U.S.A.

SECTION VI
PARTS LIST

6.1 Introduction

The illustrated parts list provides information for identifying and ordering the parts necessary to maintain the unit in peak operating condition.

The parts list also illustrates disassembly and assembly relationships of parts.

6.2 Description of Columns

The *Item* column of the parts list gives a component its own unique number. The same number is given to the component in the parts illustration. This allows a part number of a component to be found if the technician can visually spot the part on the illustration. The technician simply finds the component in question on the illustration and notes the item number of that component. Then, he finds that item number in the parts list. The row corresponding to the item number gives the technician the part number, a description of the component, and quantity of parts per subassembly. Also, if a part number is known, the location of that component can be determined by looking for the item number of the component on the illustration.

The *Part No.* column lists the MIDMARK part number for that component.

The *Description* column provides a physical description of the component.

The *Qty.* column lists the number of units of a particular component that is required for the subassembly. The letters “AR” denote “as required” when quantities of a particular component cannot be determined, such as: adhesive.

Bullets { • } in the *Part No.* column and the *Description* column show the indenture level of a component. If a component does not have a bullet, it is a main component of that illustration. If a component has a bullet, it is a subcomponent of the next component listed higher in the parts list than itself that does not have a bullet. Likewise, if a component has two bullets, it is a subcomponent of the next component listed higher in the parts list than itself that has only one bullet.

6.3 Torque Specifications and Important Assembly Notes

When specific assembly torque specifications, measurements, or procedures have been identified, by our engineering department, as required to assure proper function of the unit, those torque specifications measurements, and procedures will be noted on the parts illustrations. Adherence to these requirements is essential.

© Midmark Corporation 2002 SF-1831

Printed in U.S.A.

M9 / M11 Sterilizer Printer

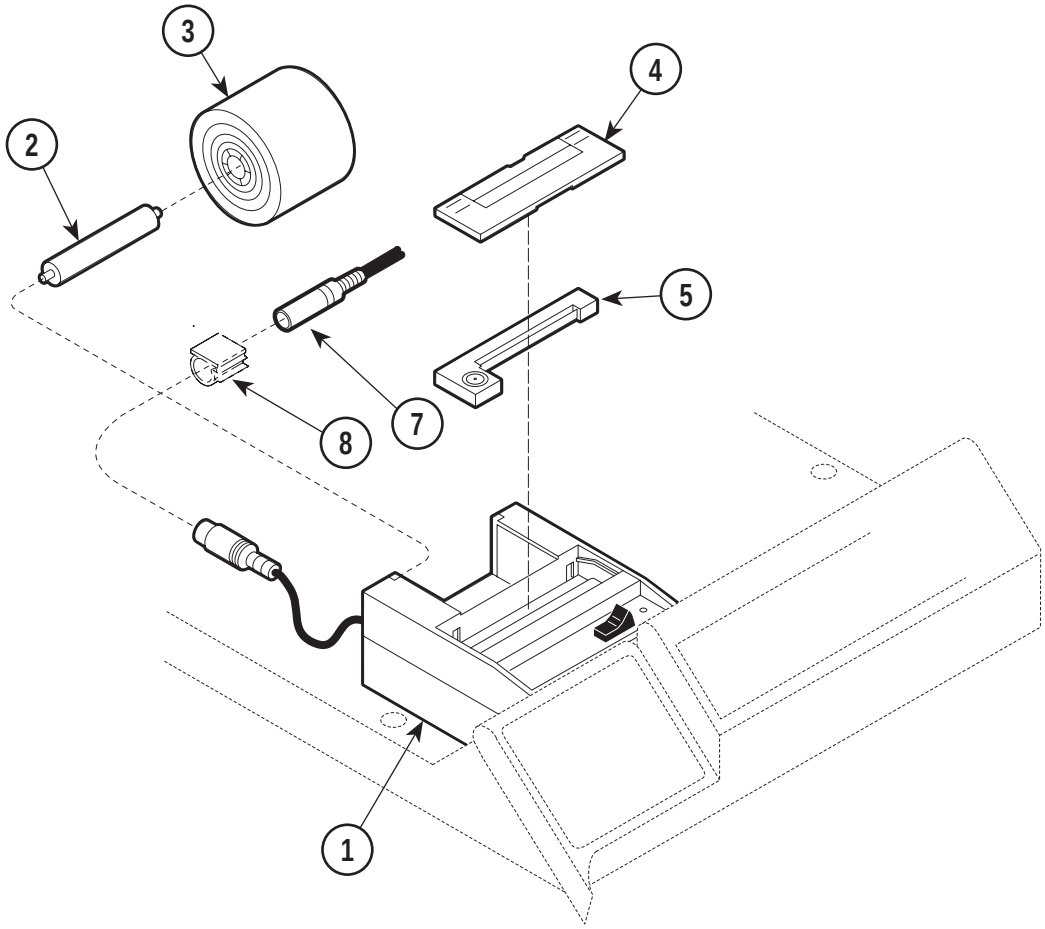

MA203302

Used on sterilizers with the serial number prefix; CZ, DA, DB, DX, DY, FD, FF, FG, FK, FL, FP, FR, FS, FT, FX, FY, GB, GC, GD, LA, OM and TFN

Item	Part No.	Description	Qty.
	9A155001	Sterilizer Accessory Printer (Includes Items 1 thru 8 plus packaging)	1
1	•	• Printer	Ref
2	• 053-0506-00	• Arbor	1
3	• 060-0008-00	• Paper Roll	1
4	• 053-0507-00	• Cover	1
5	• 053-0505-00	• Printer Cartridge	1
6	• 002-0371-00	• Cartridge/Paper Kit (Includes Two Rolls of Paper and One Cartridge	1
7	• 015-0978-00	• Printer Wiring Harness	1
8	• 053-0389-01	• Printer Harness Clip	1

Always Specify Model & Serial Number

© Midmark Corporation 2002 SF-1831

Printed in U.S.A.

M11 Cassette Rack Assembly

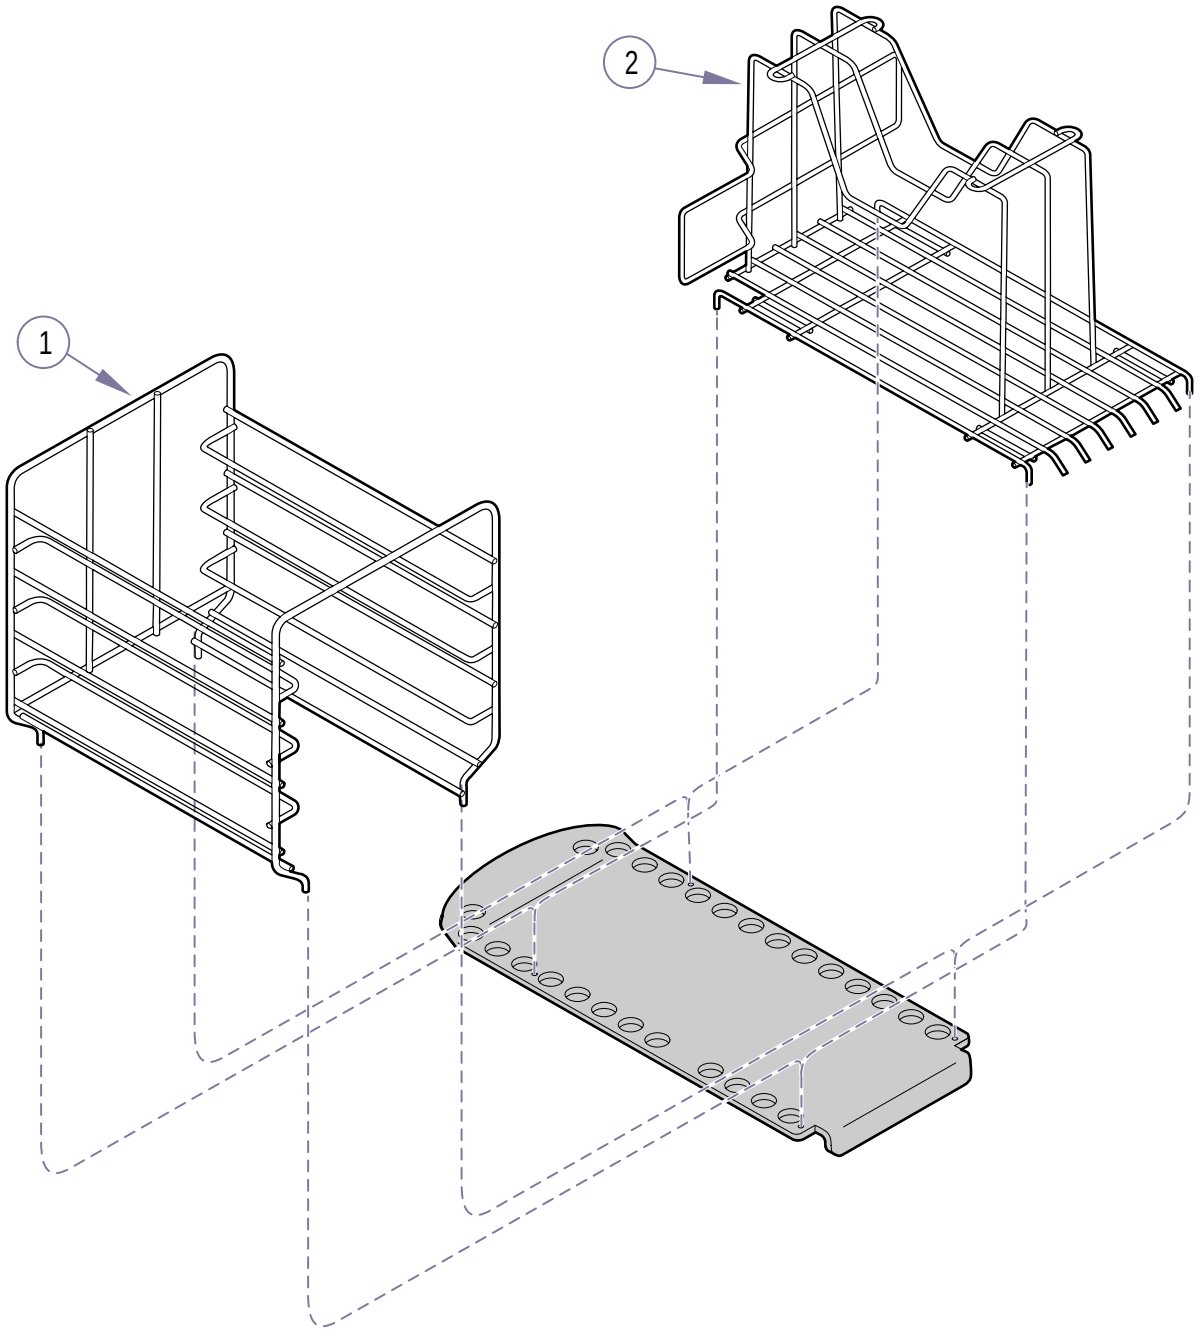

MA604400i

Used on sterilizers with the serial number prefix; FP, FR, FS, FT, GB, GC and GD

Item	Part No.	Description	Qty.
	9A215001	M11 Horizontal Cassette Rack (Includes Item 1 plus packaging)	1
	9A215002	M11 Vertical Cassette Rack (Includes Item 2 plus packaging)	1

Item	Part No.	Description	Qty.
1	030-0978-00	M11 Horizontal Cassette Rack	1
2	030-1077-00	M11 Vertical Cassette Rack	1

Always Specify Model & Serial Number

© Midmark Corporation 2002 SF-1831

Printed in U.S.A.

Deep Tray Assembly (M9)

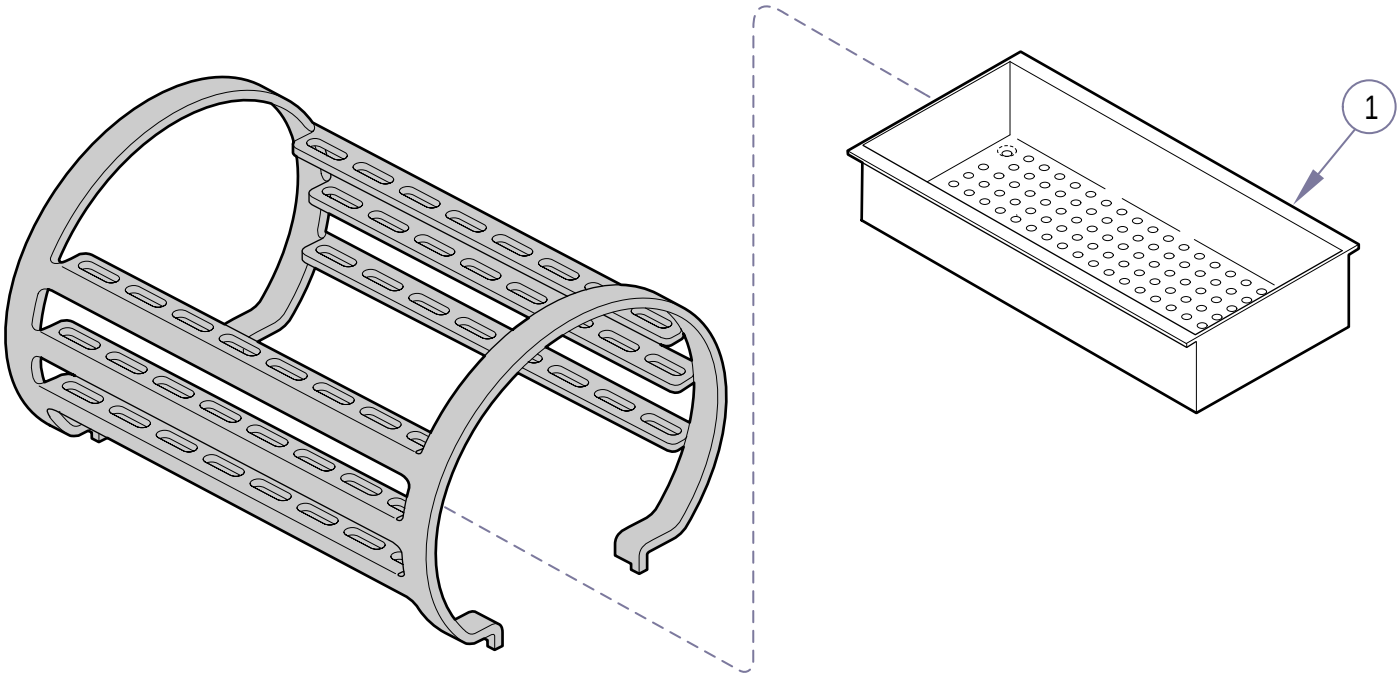

MA604500i

Used on sterilizers with the serial number prefix;
CZ, DA, DB, DX, DY, FD, FF, FG,FK, FL, FX, FY, LA, OM and TFN,

Item	Part No.	Description	Qty.
	9A224001	M9 Sterilizer Deep Tray (Includes Items 1 plus packaging)	1

Item	Part No.	Description	Qty.
1	• 050-3551-00	• M9 Deep Tray	1

Always Specify Model & Serial Number

© Midmark Corporation 2002 SF-1831

Printed in U.S.A.

Deep Tray Assembly (M11)

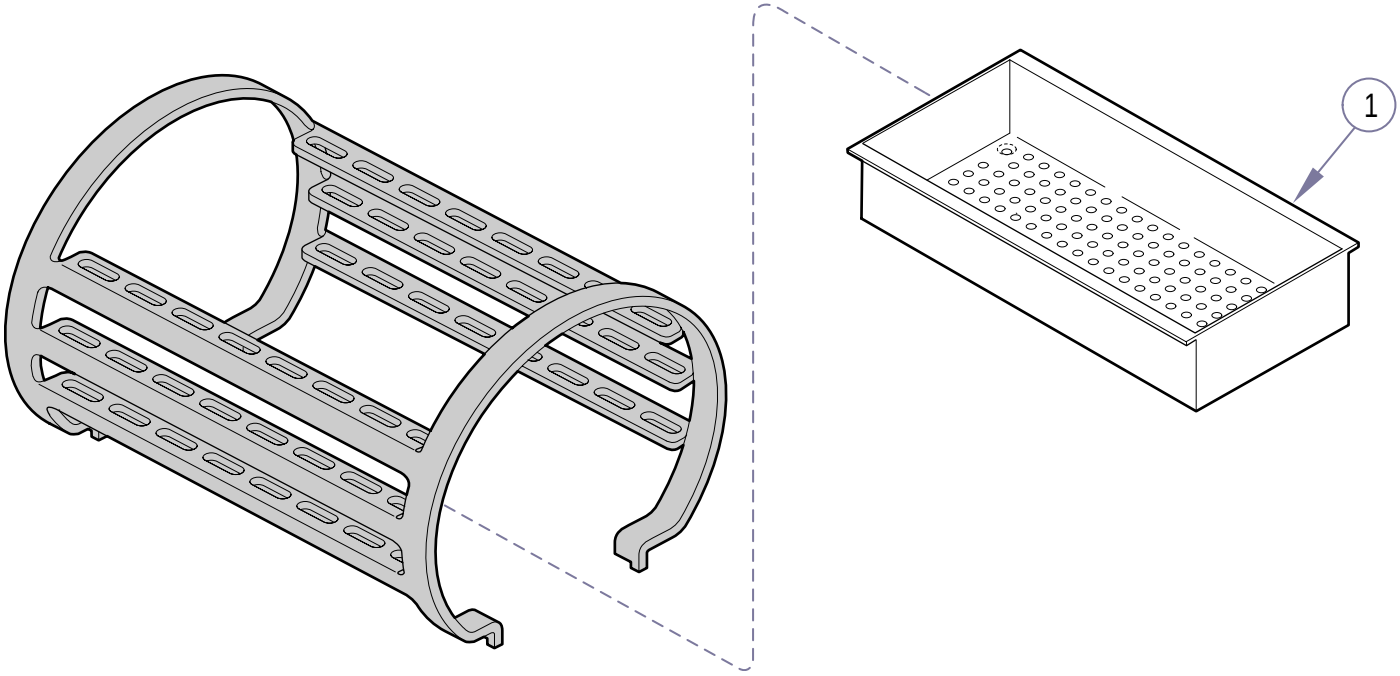

MA604500i

Used on sterilizers with the serial number prefix; FP, FR, FS, FT, GB, GC and GD

Item	Part No.	Description	Qty.	Item	Part No.	Description	Qty.
	9A225001	Accessory Printer (Includes Items 1 plus packaging)	1	1	• 050-3552-00	• M11 Deep Tray	1

Always Specify Model & Serial Number

© Midmark Corporation 2002 SF-1831

Printed in U.S.A.

Pouch Rack (M9 / M11)

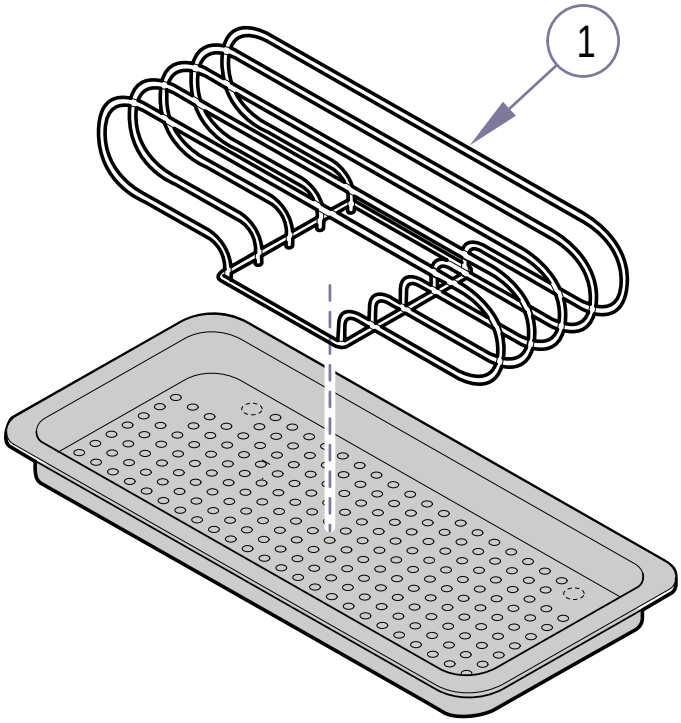

MA604700i

Used on sterilizers with the serial number prefix; CZ, DA, DB, DX, DY, FD, FF, FG, FK, FL, FP, FR, FS, FT, FX, FY, GB, GC, GD, LA, OM and TFN

Item	Part No.	Description	Qty.	Item	Part No.	Description	Qty.
	9A226001	Accessory Printer (Includes Items 1 plus packaging)	1	1	• 030-1017-00	• Passive Pouch Rack	1

Always Specify Model & Serial Number

© Midmark Corporation 2002 SF-1831

Printed in U.S.A.

Pouch Rack (M4.9)

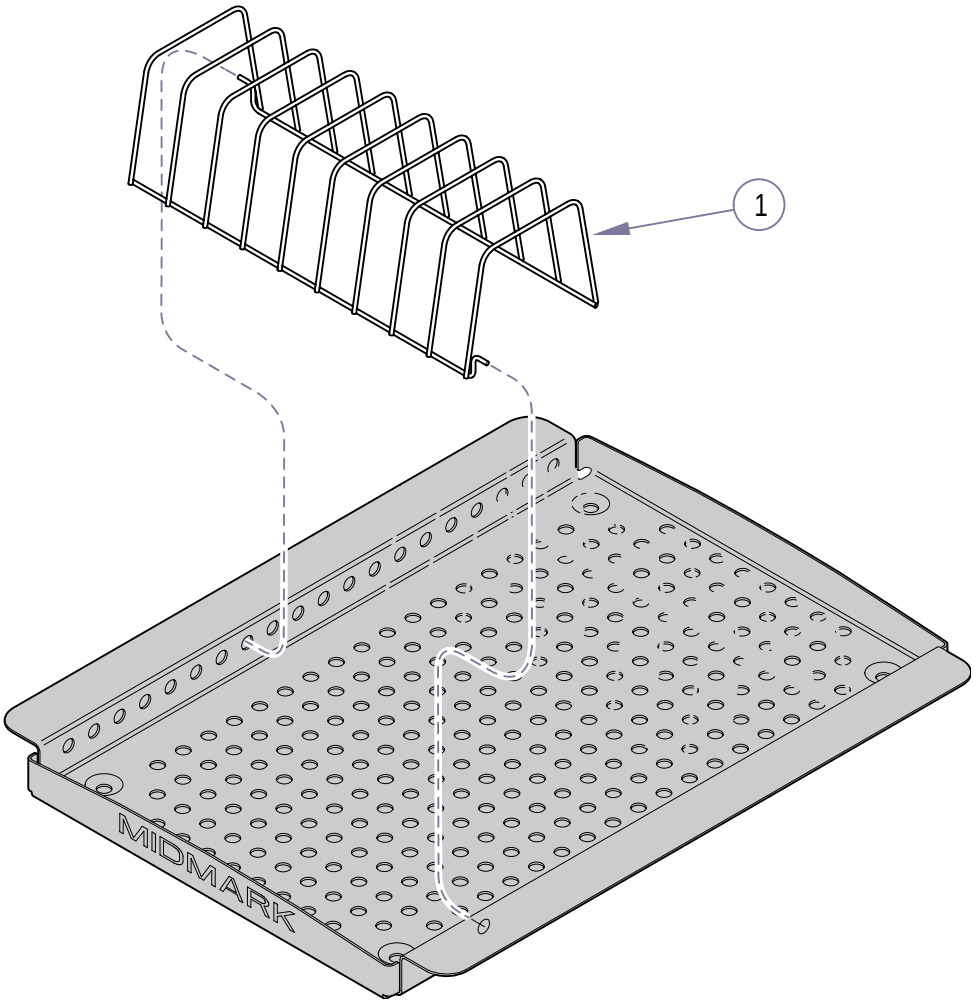

MA587101i

Used on Sterilizers with the serial number prefix; LT1000, LV1000 thru present

Item	Part No.	Description	Qty.
	9A258001	M4.9 Sterilizer Pouch Rack (Includes Items 1 and 2 plus packaging)	1
1	• 003-1253-00	• M4.9 Pouch Rack Instruction Sheet	1
2	• 030-1163-00	• M4.9 Pouch Rack Weldment	1

Always Specify Model & Serial Number

© Midmark Corporation 2002 SF-1831

Printed in U.S.A.

Sterilizer Printer (M4.9, New M9, New M11)

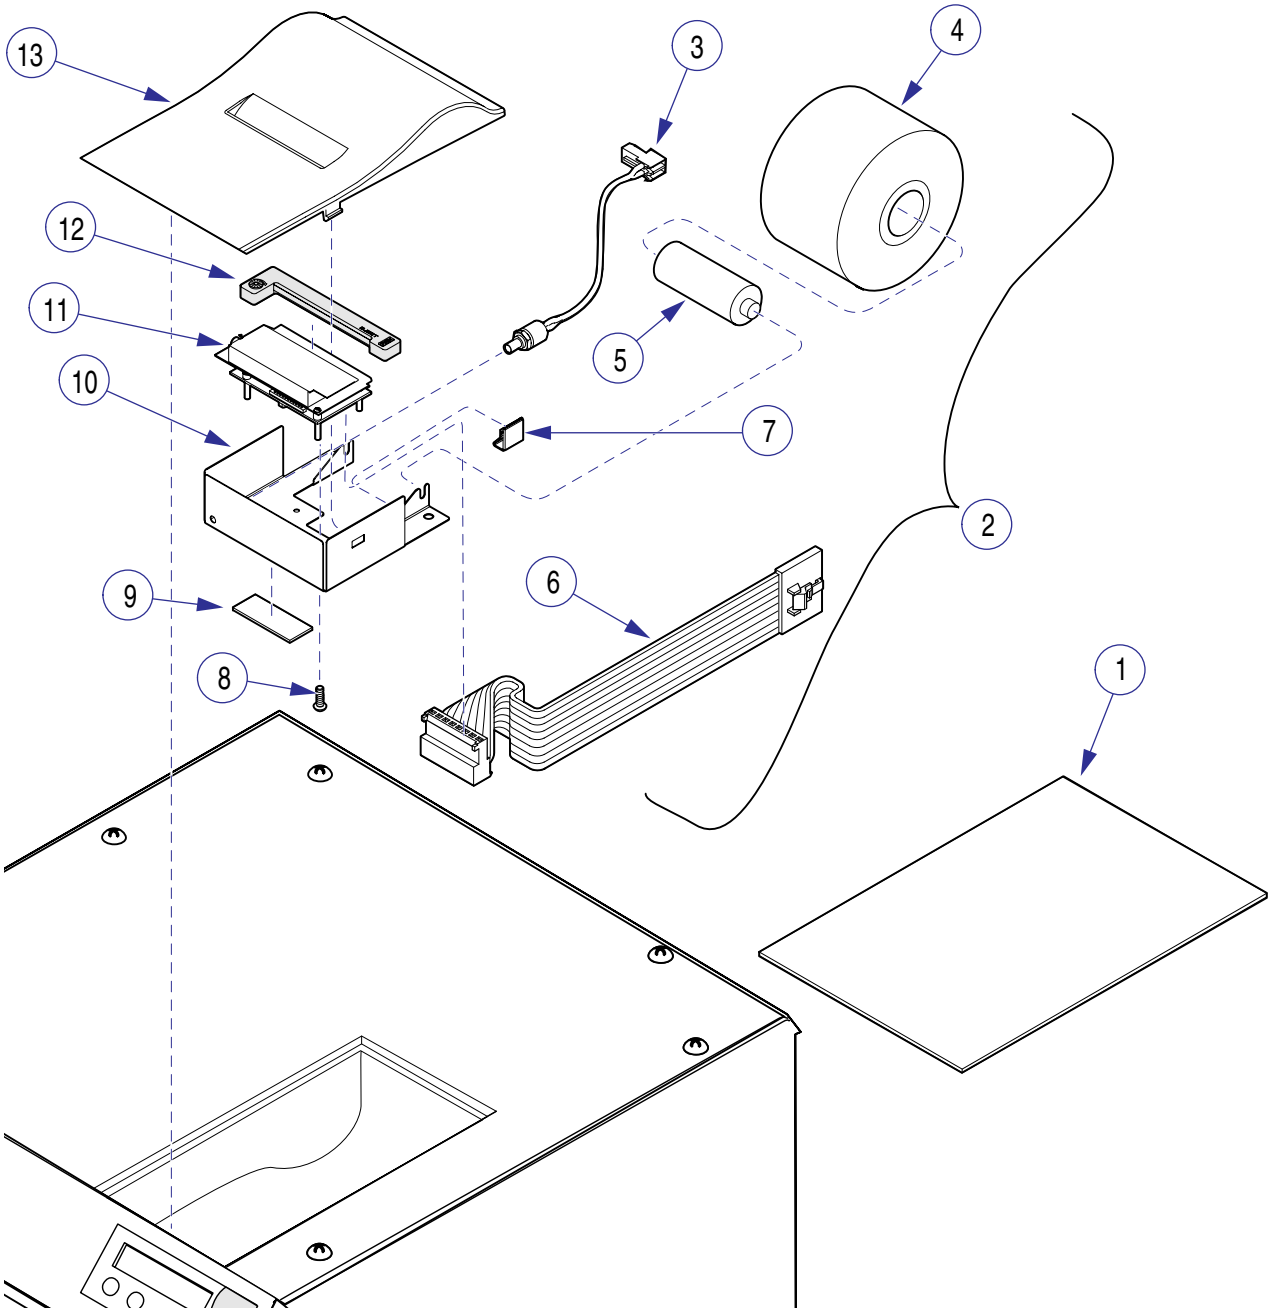

MA502101ii

Used on Sterilizers with the serial number prefix; LT1000, LV1000 thru present

Item	Part No.	Description	Qty.
	9A259001	Sterilizer Printer Accessory (Includes Items 1 and 2 plus packaging)	1
1	• 003-1194-00	• Printer Installation Instructions	Ref
2	• 029-2229-00	• Printer Assembly (Includes Items 3 thru 13)	Ref
3	• • 015-1323-00	• • Printer Feed Cable	1
4	• • 060-0008-00	• • Paper Roll	1
5	• • 053-0506-00	• • Paper Roll Spindle	1
6	• • 015-1529-00	• • Printer Ribbon Cable Assembly	1
7	• • 053-1231-00	• • Flat Wire Cable Clamp	1
8	• • 040-0002-07	• • Screw	4
9	• •	• • Serial Number Label	Ref
10	• • 050-5011-00	• • Printer Bracket	1
11	• • 015-1752-00	• • Printer	1
12	• • 053-0505-00	• • Printer Ribbon	1
13	• • 053-0927-00	• • Printer Cover	1

Always Specify Model & Serial Number

© Midmark Corporation 2002 SF-1831 (Rev. 9/03)

Printed in U.S.A.

External Condensing Tank

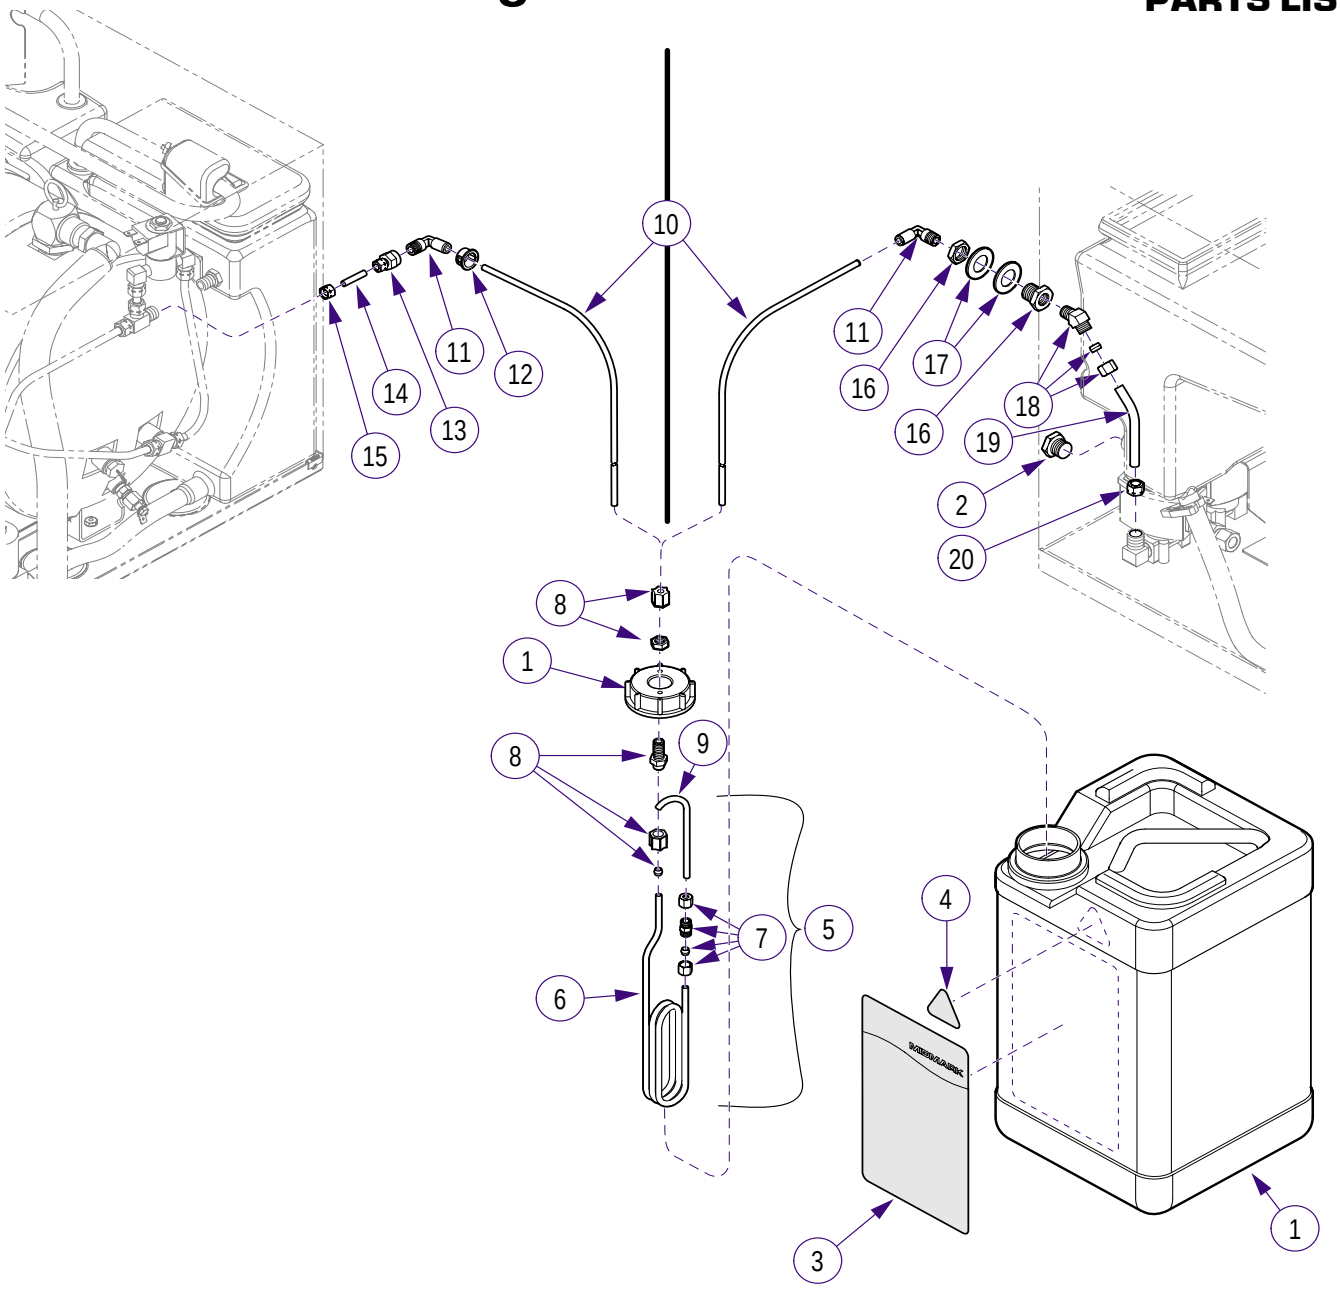

MA576902i

Used on Sterilizers with the serial number prefix;LT1000, LV1000, RN1000, RP1000, RR1000, RS1000, RT1000, RV1000, RW1000, RX1000, RY1000, RZ1000 thru present

Item	Part No.	Description	Qty.
	9A260001	External Condensing Tank Accessory (M9,M9D, M11, & M11D Includes Items 1 thru 17) M4.9 (Includes Items 1 thru 12 and 17 thru 23)	
1	• 053-1014-01	• External Condensing Tank	1
2	• 014-0344-00	• Plug	1
3	• 061-0738-00	• External Condensing Tank Label	1
4	• 061-0726-00	• Hot Surface Label	1
5	• 029-2356-00	• External Condensing Tank Coil Assembly (Includes Items 3 thru 5)	1
6	• • 014-0330-00	• • External Condensing Coil	1
7	• • 014-0352-00	• • 1/4" Male Connector	1
8	• •014-0350-00	• • Plastic Bulkhead Union	1
9	• • 014-0351-00	• • External Condensing Coil Spout	
10	• 053-0390-00	• Tubing (60" Length)	AR
11	• 014-0341-02	• 90° Elbow Push Connector	1
12	• 053-0068-11	• Snap Bushing	1
13	• 014-0383-01	• Female Connector	1
14	• 014-0424-00	• Tube	1
15	• 014-0392-00	• Sleeve Compresion Nut	1
16	• 014-0209-01	• Bulkhead Coupling	1
17	• 045-0001-112	• Washer	2
18	• 014-0201-00	• 45° Male Elbow	1
19	• 014-0394-00	• External Vent Tube	1
20	• 014-0392-01	• Compression Nut / Sleeve Assembly	1

Always Specify Model & Serial Number

© Midmark Corporation 2002 SF-1831 Rev 6/03

Large Cassette Tray (M11)

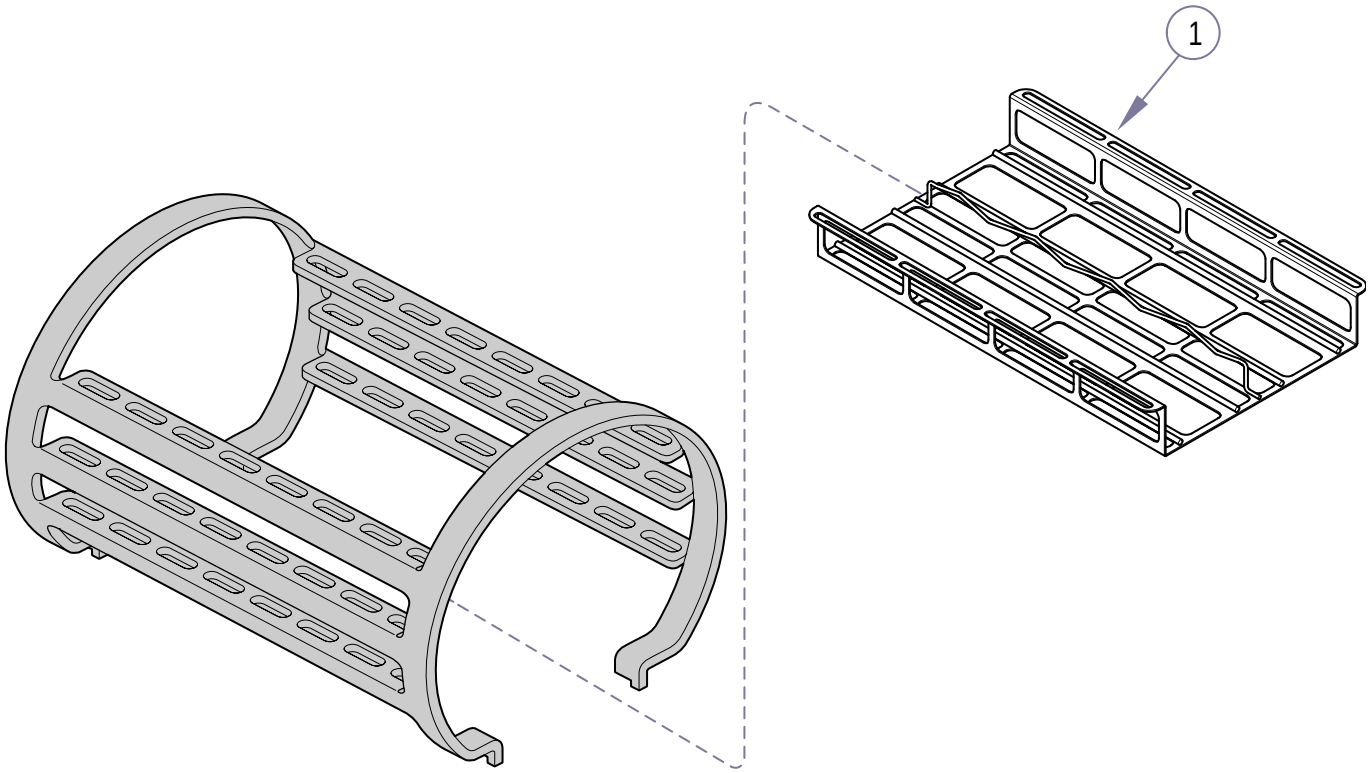

MA604600i

Used on sterilizers with the serial number prefix; FP, FR, FS, FT, GB, GC and GD

Item	Part No.	Description	Qty.
	9A306001	M11 Large Cassette Tray (Includes Items 1 and packaging)	1
1	• 030-1290-00	• M11 Large Cassette Tray Weldment ...	1

Always Specify Model & Serial Number

© Midmark Corporation 2002 SF-1831

Printed in U.S.A.

Tray and Cassette Tool (M4.9 / M9 / M11)

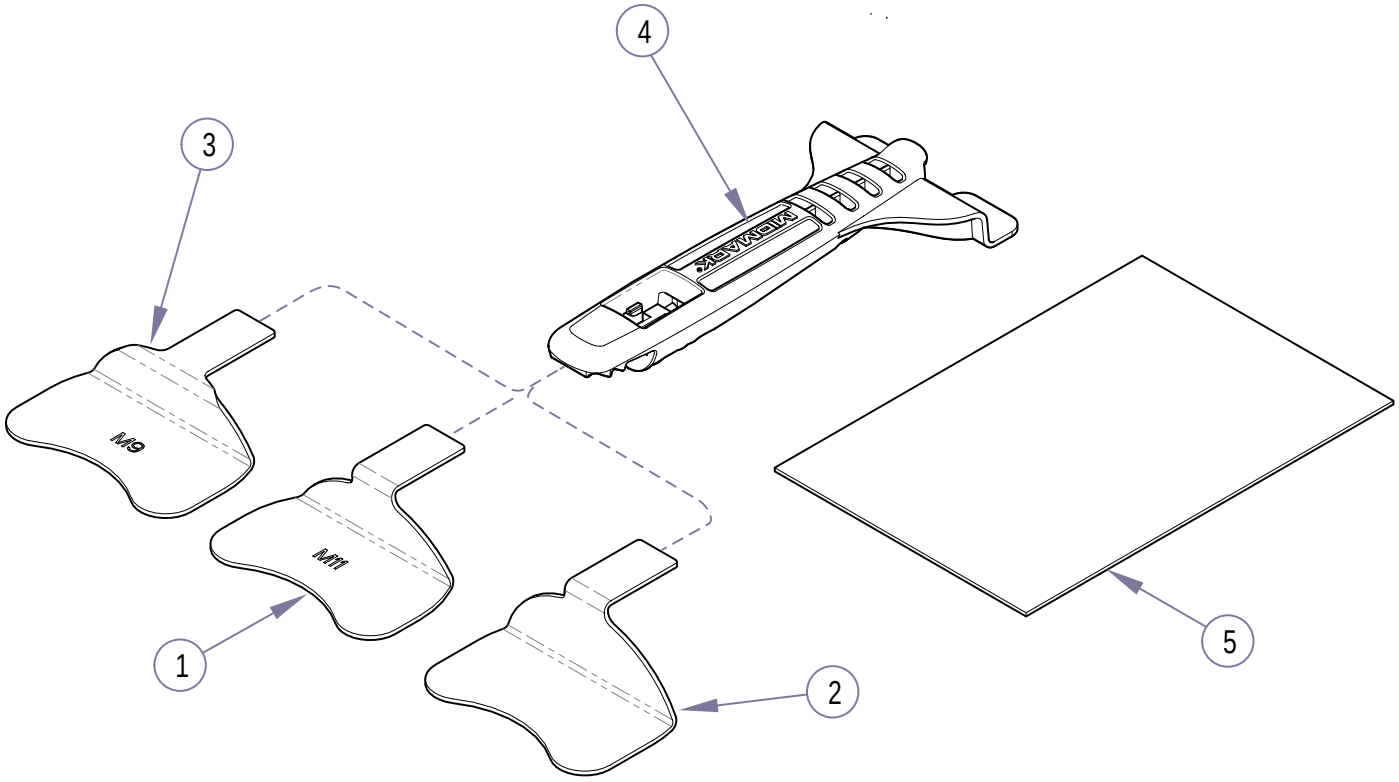

MA604800i

Used on sterilizers with the serial number prefix; CZ, DA, DB, DX, DY, FD, FF, FG, FK, FL, FP, FR, FS, FT, FX, FY, GB, GC, GD, LA, LT, LV, OM and TFN

Item	Part No.	Description	Qty.	Item	Part No.	Description	Qty.
	9A307001	Tray and Cassette Tool	1	3	• 050-4660-02	• M9 Tray Plate	1
1	• 050-4660-00	• M11 Tray Plate	1	4	• 053-1038-00	• Tray / Cassette Tool	1
2	• 050-4660-01	• Cassette Plate	1	5	• 003-1218-00	• Tray Tool Instructions	1

Always Specify Model & Serial Number

© Midmark Corporation 2002 SF-1831

Printed in U.S.A.

Return To Table Of Contents

COMMENTS

The Technical Publications Department of Midmark Corporation takes pride in its manuals. We are sure that our manuals will fill all your needs when you are performing scheduled maintenance, servicing, or repairs on a Midmark product. However, if you find any errors or feel there should be a change, addition, or deletion to the manuals, please let us know. We will correct any errors that we are made aware of and we will review requests for changes, additions, or deletions to the manuals and incorporate those requests deemed appropriate.

If you see something in one of our manuals that you like or dislike, please let us know. Also, if there is something you feel we could do to produce a better manual, please let us know.

If an error is found, please list the page and paragraph/figure in which the error was found along with a brief description of what the error is. If the correction to the error is known, please include that information also. If a change, addition, or deletion is being requested, please list the page and paragraph/figure needing the change, along with a brief description of how you feel the paragraph/figure should be changed.

Page	Paragraph/Figure	Description

Please fax or mail a copy of this completed comment sheet to:

Midmark Corporation
ATTN: Technical Publications Dept.
60 Vista Drive
Versailles, Ohio 45380
Fax: (937) 526-5542

© Midmark Corporation 1994 Rev. 8/96

Printed in U.S.A.

Return To Table Of Contents

FAX ORDERING FORM

(SERVICE PARTS ONLY)

NOTES:

- **ALL BLOCKED AREAS MUST BE COMPLETED.**
- **USE FOR NON-WARRANTY FAX ORDERS ONLY. WARRANTY ORDERS MUST BE TELEPHONED IN (1-800-MIDMARK).**
- **ORDER MUST MEET $35.00 MINIMUM.**

SHADED AREAS TO BE FILLED OUT BY MIDMARK PERSONNEL ONLY.

REP #: _____ **DISCOUNT %:** _____ **DATE:** _____

CAT #: _____ **TECHNICIAN:** _____ **TIME:** _____

ATTENTION: SERVICE DEPARTMENT FAX#: 877-249-1793

ACCT #: _____ **P.O. #:** _____ **DATE:** _____

NAME: _____ **SHIP TO:** _____

ADDRESS: _____

CITY, ST.: _____

CONTACT: _____

PHONE: _____

☐ **NON-EMERGENCY ORDER - TO SHIP WITHIN 72 HOURS IF PART(S) IN STOCK.**

☐ **EMERGENCY ORDER - TO SHIP WITHIN 24 HOURS IF PART(S) IN STOCK (IF ORDER IS RECEIVED BEFORE 1:30 P.M. E.S.T).**

SEND NOTIFICATION IF PARTS ARE NOT AVAILABLE TO SHIP WITHIN 24 HOURS VIA E-MAIL OR FAX TO: _____

METHOD OF SHIPMENT **OTHER** _____

UPS	FED EX
☐ NEXT DAY A.M.	☐ NEXT DAY A.M.
☐ NEXT DAY P.M.	☐ NEXT DAY P.M.
☐ 2ND DAY	☐ 2ND DAY
☐ GROUND	☐ ECONOMY

FA ___
ADD ___

QTY.	PART #	DESCRIPTION (SPECIFY COLOR OF ITEM IF APPLICABLE)	COLOR CODE	PRICE/PER
	SPECIAL CODES:		**TOTAL COST: $**	

© Midmark Corporation 2000

Printed in U.S.A.

Return To Table Of Contents

MIDMARK®

Midmark Corporation, Versailles, Ohio 45380 U.S.A.
937-526-3662 FAX 877-249-1793

Return To Table Of Contents

Subject To Change Without Notice

© Midmark Corporation Rev. 8/96

Printed in U.S.A.